

## Single-Phase AC/DC Power Meter




## High-accuracy measurement of standby to operating power

- Wide measurable range : 10  $\mu$ A to 30 A, 60 mV to 1000 V
- Basic accuracy for voltage, current and power :  $\pm 0.1\%$ \*
- Frequency bandwidth : DC, 0.1Hz to 100kHz
- High-accuracy measurement even for equipment with low power factors :  $\pm 0.1\%$  f.s. power factor effect
- Standby power consumption : Built-in harmonic measurement; IEC62301-compliant
- Measure up to 5000A AC : Built-in external sensor input terminals (PW3335-03, -04)

\* For complete details, please refer to the specifications.

# Single-Phase Power Meter with All-Round Capability

High accuracy of  $\pm 0.1\%$ \*<sup>1</sup> and guaranteed accuracy range from 1 to 150% f.s.

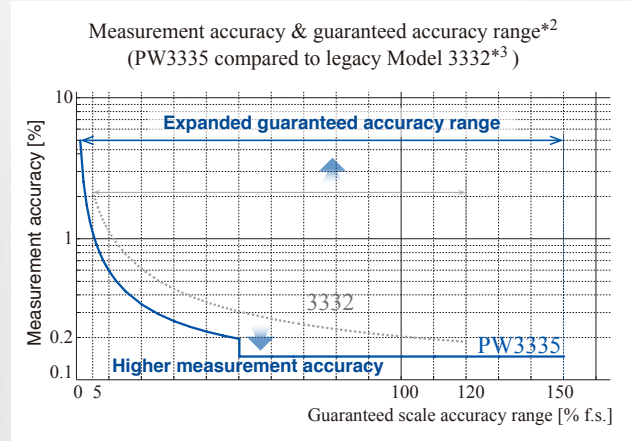

\*2 : Up to 1000 V with a voltage range of 1000 V.  
 \*3 : For detailed specifications of Model 3332, see the comparison chart on page 6.

**Power Meter PW3335:** Single-phase AC/DC power meter with built-in harmonic measurement  
**Voltage range:** 6.0000 V to 1.0000 kV  
**Current range:** 1.0000 mA to 20.000 A (30 A maximum)

With an expanded guaranteed accuracy range, the power meter minimizes range switchings even under power fluctuations.

## Standby power

\*1 : For complete details, please refer to the specifications.

DC, 0.1Hz to 100kHz frequency bandwidth  
 With built-in harmonic measurement for detailed analysis

Measure the standby power of AC adapters, both primary-side AC and secondary-side DC



Measure power supply conversion devices such as inverters and thyristors



Measures solar panels and power converters, max. 1000V range



### Measured power parameters

Voltage	Current	Effective power	Apparent power
Reactive power	Power factor	Phase angle	Frequency
Integral current	Effective integral power	Waveform peak value	Crest factor
Maximum current ratio	Time-averaged current	Time-averaged effective power	Ripple rate

### Harmonic measurement parameters

Harmonic effective value	Harmonic effective power	Total harmonic distortion	Fundamental wave effective value
Fundamental wave effective power	Fundamental wave apparent power	Fundamental wave reactive power	Fundamental wave power factor (displacement power factor)
Fundamental wave voltage/current phase difference	Harmonic wave content		
Harmonic voltage phase angle*	Harmonic current phase angle*	Harmonic voltage/current phase difference*	

\*: Only with PC communication

Use in the development and production of solar panels and AC adapters, secondary-side DC equipment and inverters, and power converters such as thyristors. Equipped with multiple functions for computing a wide variety of items, the PW3335 Power Meter can also be used alone for detailed analysis.

# from AC/DC Standby to Operating Power

# PW3335

Highest basic accuracy and DC accuracy of any instrument in its class

**±0.1%**\*


Thanks to Hioki's accumulated technology and track record, the PW3336/PW3337 delivers the highest basic accuracy and DC accuracy of any instrument in its class. Reliable measurement accuracy ensures robust performance in customers' measurement applications.

\* For complete details, please refer to the specifications.




Greater accuracy for standby power

The PW3335 Power Meter delivers a range configuration that lets you measure extremely low power levels with a margin to spare. Accuracy can be set from 10 μA and up for current, and 0 W and up for effective power. Perfect for measurements according to IEC62301 and other standards.



Peak value of up to 600% of the range, supporting crest factor of 6

Current waveforms in the switching power supply or at the primary-side of inverters become steep and often exceeds the fundamental range, preventing them from being accurately measured. The PW3335 resolves these issues by offering a crest factor of 6, allowing it to measure accurately even when the waveform peaks are high relative to its range.

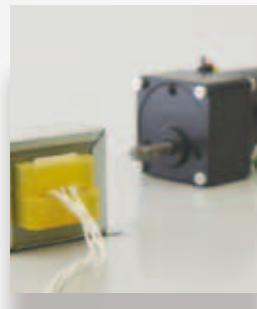


Power factor effects of no more than ±0.1% f.s.

The effective power value may be affected in situations with low power factors, such as measurement of standby power or unloaded operation of transformers and motors. The PW3335 reduces the power factor effect to less than a half of that available in legacy models.

Power data and harmonic data — all measured simultaneously




Example of half-wave rectification waveform



All measurement data are internally processed in parallel simultaneously. Even when waveforms have mixed AC/DC components — half-wave rectification waveforms for example — the individual components can be measured simultaneously. The PC communication application further enables 180 or more measurement parameters to be acquired simultaneously.



Example of distorted waveform containing harmonic component




Built-in harmonic measurement

The PW3335 measures harmonics up to the 50th order. Use it for evaluation and development of power sources for home appliances and other electrical equipment. Simultaneously display the effective voltage and total harmonic distortion (THD) on the screen. For THD computation, any maximum harmonic order can be specified.

Power consumption and regeneration (recharging) power integrated separately



Example of power fluctuation




Use for evaluating the input and output of secondary batteries in EVs, etc., and for measuring the sold power of solar panels. Power consumption and regeneration (recharging) power can each be measured separately.

Power consumption Wh(+)  
Regeneration power Wh(-)



MAX/MIN hold function for spotting current peaks at a glance

Capture maximum and minimum values such as inrush current waveform peak values and maximum consumed power.

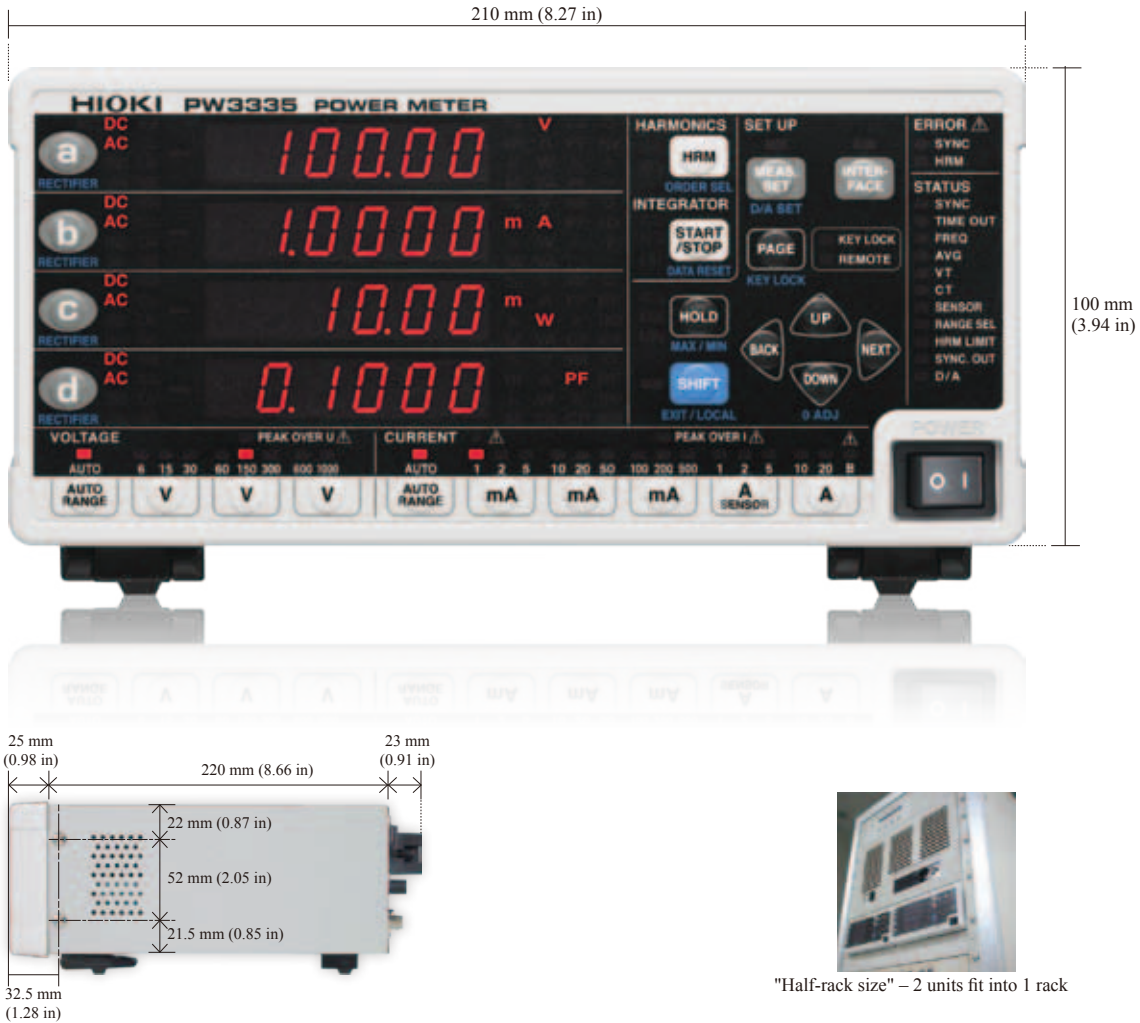

# Diverse and Powerful Functionality

## Measure power in accordance with international standards

The PW3335 is engineered to comply with important international standards, including IEC62301 for electrical power consumption in standby mode and the ErP Directive or Energy Star standard. It can also be used to find the special parameters required by the standards – such as THD, CF, and MCR.

### THD (total harmonic distortion)


Indicates the total harmonic components in an AC waveform.

### CF (crest factor)

Also known as the peak-to-rms ratio, the ratio of the waveform's peak value to its effective value.

### MCR (maximum current ratio)

Evaluation index of the current, calculated from the crest factor and the power factor.



Download free software for creating IEC62301-compliant reports from the Hioki website.

## Measure integral power of equipment that operates intermittently or has a large power variation

### Time-averaged effective integral power

Use this feature to measure the power of equipment that operates intermittently or is under cycle control. Average power is calculated from the integral value of the fluctuating power.




Example of intermittent operation




Example of cycle control

### Auto-range integration

A function whereby the device jumps automatically to the optimal current range for the consumed current as it measures and integrates the values. Power integration can be carried out on separate ranges, enabling measurements for individual modes in equipment that has fluctuations in power levels.

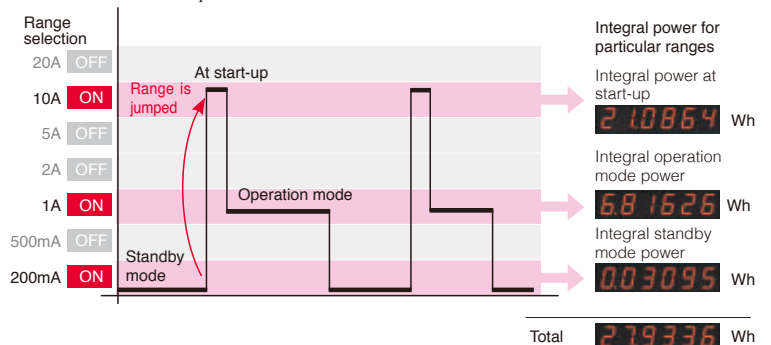

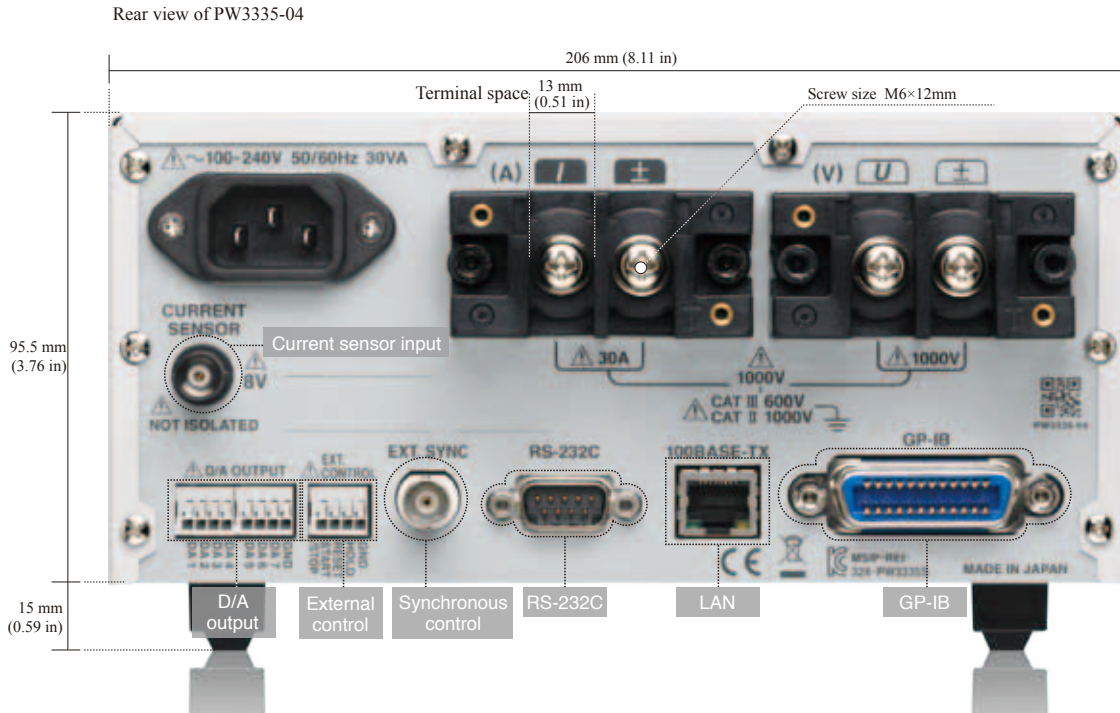

Models and available functions

Model	Harmonics measurement	Synchronous control	LAN	RS-232C	GP-IB	D/A output	Current sensor input
PW3335	✓	✓	✓	✓	—	—	—
PW3335-01	✓	✓	✓	—	✓	—	—
PW3335-02	✓	✓	✓	✓	—	✓	—
PW3335-03	✓	✓	✓	✓	✓	—	✓
PW3335-04	✓	✓	✓	✓	✓	✓	✓

✓ : available  
— : not available

## Rich interfaces and extensibility

**Waveform output**

**High-speed level output**  
Single-cycle updating

**Level output**  
200ms updating

### 3 D/A output types (PW3335-02, PW3335-04)

The PW3335 can output measurement values to a data logger, Hioki Memory HiCorder or similar, via voltage signals. The power meter is also built in with functions for outputting the high-speed level of each successive fundamental wave cycle\*, in addition to instantaneous waveform output and level output, and provides in-depth analysis of power-consuming equipment such as cutting/grinding tool monitoring equipment.

\* For voltage and current, cycle-by-cycle updating is possible only with an input of 45 to 66 Hz.




### PC communication software

By using the bundled PC application, you can control the power meter from a PC without needing to code your own communication program. The software enables you to save data to the PC, display waveforms, and perform efficiency calculations\*, etc.

Compatible with LAN, RS-232C, GP-IB

\*Two or more PW3335s are necessary in order to carry out efficiency computation.



Synchronous control cable 9165

### Up to 8 units of simultaneous control

Use the simultaneous control feature for measuring input/output efficiency of the power source equipment, for making comparisons between multiple equipment, or for simultaneous parallel testing of production lines and achieve measurement with guaranteed synchronization. Efficiency computation is also possible in conjunction with PC software. Synchronization with both the Hioki PW3336 and PW3337 Power Meters is also supported.




### Pair with current sensors delivering a maximum accuracy of ±0.26% to measure 30 A and up (PW3335-03, PW3335-04)

You can input up to 5000A AC with the use of an optional current sensor. Using Hioki AC/DC high-accuracy pull-through sensors will enable precise measurement with maximum accuracy of ±0.26%.


## 6 PC Communication Software – PW Communicator

PW Communicator is an application software for communicating between a PW3335 series power meter and a PC. Free download is available from the Hioki website. The application contains convenient functions for setting the PW3335, monitoring the measurement values, acquiring data via communication, computing efficiency, and many more.

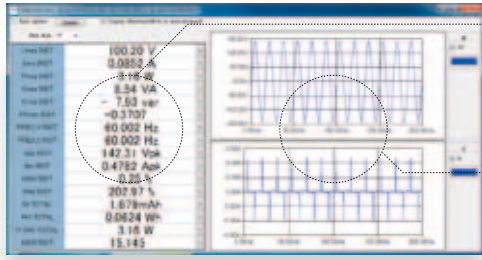

### Value monitoring

The Value monitoring function displays the PW3335's measurement values on the PC screen. You can freely select up to 64 values, such as voltage, current, power, and harmonics.

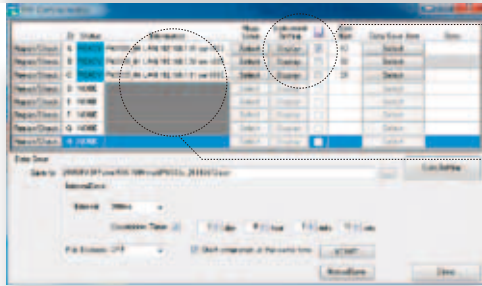


### Waveform monitoring

This function enables you to monitor the voltage, current, and waveforms measured by the meter right on the PC screen.

### Meter setting

The application also enables you to configure the connected PW3335 from the PC screen.

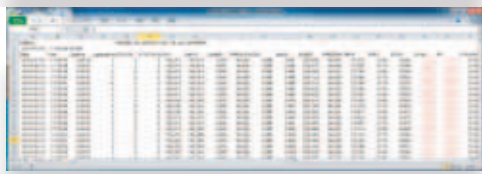

### Synchronous measurement

When using multiple PW3335s, computation of the input/output efficiency of a power converter and similar operations are supported. This feature can be used to synchronously control up to 8 meters – including Hioki PW3336 and PW3337 series units – connected together with synchronous control cables.

### Saving data as CSV file

Record 180 or more measurement data to a CSV file at fixed intervals. The shortest interval between recordings is 200 ms.

### PW Communicator Specifications

Availability	Free download from the Hioki website
Operating environment	PC/AT-compatible
OS	Windows 8, Windows 7 (32/64-bit)
Memory	2GB or more recommended
Interface	LAN, RS-232C, GP-IB

## IEC62301-compliant reporting software

Download free software for creating IEC62301-compliant reports from the Hioki website.

## LabVIEW Driver

A LabVIEW driver compatible with the PW3335 will enable you to acquire data and build measurement systems. (LabVIEW is a registered trademark of National Instruments Corporation.)

## Comparison with Hioki legacy Model 3332

	PW3335 series	3332
Frequency bandwidth	DC, 0.1 Hz to 100 kHz	1 Hz to 100 kHz
Sampling	700 kHz digital sampling	Analog computation
Voltage measurement range	6 V to 1000 V	15 V to 600 V
Current measurement range	1 mA to 20 A	1 mA to 50 A
Power measurement range	Determined by combination of voltage and current ranges. 6.0000 mW and up	Determined by combination of voltage and current ranges. 15.0000 mW and up
Basic accuracy (DC)	Voltage/current/power: $\pm 0.1\%$ rdg, $\pm 0.1\%$ f.s.	-
Basic accuracy (45 Hz to 66 Hz)	Voltage/current/power: $\pm 0.1\%$ rdg, $\pm 0.05\%$ f.s.	Voltage/current/power: $\pm 0.1\%$ rdg, $\pm 0.1\%$ f.s.
Effect of power factor	$\pm 0.1\%$ f.s. with 45 Hz to 66 Hz, PF = 0	$\pm 0.23\%$ f.s. with 45 Hz to 66 Hz, PF = 0
Communication interface	LAN RS-232C (PW3335, PW3335-02, PW3335-03, PW3335-04) GP-IB (PW3335-01, PW3335-04)	RS-232C GP-IB
Synchronous control	Up to 8 meters	-
Harmonics measurement	Available on all models Compliant with IEC61000-4-7:2002	-
Current sensor support	PW3335-03, PW3335-04	-
Auto-range integration function	Available	-
D/A output	7 channels (level output, high-speed level output and waveform output selectable)	Level output (fixed voltage, current and effective power) Waveform output (fixed voltage and current) 1-channel D/A level output
Time-averaged effective integral power	Computable	-
Maximum current ratio (MCR)	Computable	-

# Specifications

## Input Specifications

Measurement line type	Single-phase 2-wire(1P2W)			
Input methods	Voltage Isolated input, resistive voltage divider method Current Isolated input, shunt input method			
Voltage measurement ranges	AUTO/ 60.000 V/ 1.0000 kV	6.0000 V/ 150.00 V/ 300.00 V/	15.000 V/ 300.00 V/ 600.00 V/	30.000 V/ 600.00 V/
Current measurement ranges	AUTO/ 10.000 mA/ 100.00 mA/ 200.00 mA/ 5.0000 A/	1.0000 mA/ 20.000 mA/ 500.00 mA/ 10.000 A/	2.0000 mA/ 50.000 mA/ 1.0000 A/ 20.000 A/	5.0000 mA/ 100.00 mA/ 2.0000 A/
Power ranges	Depends on the combination of voltage and current ranges; From 6.0000 mW to 20.000 kW (also applies to VA, var) The details are as below.			
Input resistance	Voltage input terminal: Approx. 2 MΩ Current input terminal: 1 mA to 100 mA range 520 mΩ or less 200 mA to 20 A range 15 mΩ or less			

## Basic Measurement Specifications

Measurement method	Simultaneous voltage and current digital sampling, zero-cross simultaneous calculation		
Sampling frequency	Approx. 700 kHz		
A/D converter resolution	16-bit		
Frequency bandwidth	DC, 0.1 Hz to 100 kHz (Values within 0.1Hz ≤ f < 10 Hz are for reference only)		
Synchronization sources	U, I, DC (fixed to 200 ms)		
Measurement items	Voltage	Current	Active power
	Apparent power	Reactive power	Power factor
Measurement items	Phase angle	Frequency	Current integration
	Active power integration	Integration time	
Measurement items	Voltage waveform peak value	Current waveform peak value	
	Voltage crest factor	Current crest factor	
Measurement items	Maximum current ratio	Time average current	
	Time average active power	Current ripple rate	
Measurement items	Voltage ripple rate		
	Harmonic parameters		
Measurement items	Harmonic voltage RMS value	Harmonic current RMS value	
	Harmonic active power	Total harmonic voltage distortion	
Measurement items	Total harmonic current distortion	Fundamental wave voltage	
	Fundamental wave current	Fundamental wave active power	
Measurement items	Fundamental wave apparent power	Fundamental wave reactive power	
	Fundamental wave power factor (Displacement power factor)		
Measurement items	Fundamental wave voltage current phase difference		
	Harmonic voltage content percentage		
Measurement items	Harmonic current content percentage		
	Harmonic active power content percentage		
Measurement items	(The following parameters can be downloaded as data via PC communication)		
	Harmonic voltage phase angle		
Measurement items	Harmonic current phase angle		
	Harmonic voltage current phase difference		
Rectifiers	AC+DC : AC+DC measurement		
	Display of true RMS values for both voltage and current		
Rectifiers	AC+DC Umn : AC+DC measurement		
	Display of average value rectified RMS converted values for voltage and true RMS values for current		
Rectifiers	DC : DC measurement		
	Display of simple averages for both voltage and current Display of values calculated by (voltage DC value) × (current DC value) for active power		
Rectifiers	AC : AC measurement		
	Display of values calculated by $\sqrt{(AC+DC \text{ value})^2 - (DC \text{ value})^2}$ for both voltage and current Display of values calculated by (AC+DC value) - (DC value) for active power		
Rectifiers	FND : Extraction and display of the fundamental wave component from harmonic measurement		
Zero-cross Filter	100 Hz: 0.1 Hz to 100 Hz 5 kHz: 0.1 Hz to 5 kHz	500 Hz: 0.1 Hz to 500 Hz 100 kHz: 0.1 Hz to 100 kHz	

Measurement accuracy	Voltage			
Voltage	Frequency ( f )	Input < 50%f.s.	50%f.s. ≤ Input < 100%f.s.	100%f.s. ≤ Input
	DC	±0.1%rdg.±0.1%f.s.	±0.1%rdg.±0.1%f.s.	±0.2%rdg.
	0.1Hz≤f<16Hz	±0.1%rdg.±0.2%f.s.	±0.3%rdg.	±0.3%rdg.
	16Hz≤f<45Hz	±0.1%rdg.±0.1%f.s.	±0.2%rdg.	±0.2%rdg.
	45Hz≤f<66Hz	±0.1%rdg.±0.05%f.s.	±0.15%rdg.	±0.15%rdg.
	66Hz≤f<500Hz	±0.1%rdg.±0.1%f.s.	±0.2%rdg.	±0.2%rdg.
Current	Frequency ( f )	Input < 50%f.s.	50%f.s. ≤ Input < 100%f.s.	100%f.s. ≤ Input
	DC	±0.1%rdg.±0.1%f.s.	±0.1%rdg.±0.1%f.s.	±0.2%rdg.
	0.1Hz≤f<16Hz	±0.1%rdg.±0.2%f.s.	±0.3%rdg.	±0.3%rdg.
	16Hz≤f<45Hz	±0.1%rdg.±0.1%f.s.	±0.2%rdg.	±0.2%rdg.
	45Hz≤f<66Hz	±0.1%rdg.±0.05%f.s.	±0.15%rdg.	±0.15%rdg.
	66Hz≤f<500Hz	±0.1%rdg.±0.1%f.s.	±0.2%rdg.	±0.2%rdg.
Active power	Frequency ( f )	Input < 50%f.s.	50%f.s. ≤ Input < 100%f.s.	100%f.s. ≤ Input
	DC	±0.1%rdg.±0.1%f.s.	±0.1%rdg.±0.1%f.s.	±0.2%rdg.
	0.1Hz≤f<16Hz	±0.1%rdg.±0.2%f.s.	±0.3%rdg.	±0.3%rdg.
	16Hz≤f<45Hz	±0.1%rdg.±0.1%f.s.	±0.2%rdg.	±0.2%rdg.
	45Hz≤f<66Hz	±0.1%rdg.±0.05%f.s.	±0.15%rdg.	±0.15%rdg.
	66Hz≤f<500Hz	±0.1%rdg.±0.1%f.s.	±0.2%rdg.	±0.2%rdg.
Conditions of guaranteed accuracy	500Hz≤f<1kHz	±0.1%rdg.±0.2%f.s.	±0.3%rdg.	±0.3%rdg.
	1kHz≤f<10kHz	±(0.03+0.07×F)%rdg.±0.2%f.s.	±(0.23+0.07×F)%rdg.	±(0.23+0.07×F)%rdg.
	10kHz≤f<50kHz	±(0.07×F)%rdg.±0.3%f.s.	±(0.3+0.07×F)%rdg.	±(0.3+0.07×F)%rdg.
	50kHz≤f<100kHz	±(0.3+0.04×F)%rdg.±0.3%f.s.	±(0.6+0.04×F)%rdg.	±(0.6+0.04×F)%rdg.
	<ul style="list-style-type: none"> <li>• Values for f.s. depend on measurement ranges.</li> <li>• "F" in the tables refers to the frequency in kHz.</li> <li>• When using the 1 mA / 2 mA range: Add ±1 μA to 0.1 Hz to 100 kHz measurement accuracy for current. Add (±1 μA) × (voltage read value) to 0.1 Hz to 100 kHz measurement accuracy for active power.</li> <li>• When using the 200 mA / 500 mA / 1 A / 2 A / 5 A / 10 A / 20 A range: Add ±1 mA to DC measurement accuracy for current. Add (±1 mA) × (voltage read value) to DC measurement accuracy for active power.</li> <li>• When using the 1 mA / 2 mA / 5 mA / 10 mA / 20 mA / 50 mA / 100 mA range: Add ±10 μA to DC measurement accuracy for current. Add (±10 μA) × (voltage read value) to DC measurement accuracy for active power.</li> <li>• When using the 200 mA / 500 mA / 1 A / 2 A / 5 A / 10 A / 20 A range: Add ±(0.02×F)% rdg. to the measurement accuracy for current and active power for which (10 kHz &lt; f ≤ 100 kHz).</li> <li>• The measurement results for following input are considered reference values: Values for voltage, current, and active power for which 0.1 Hz ≤ f &lt; 10 Hz. Values for voltage, current, and active power in excess of 220 V or 20 A for which 10 Hz ≤ f &lt; 16 Hz. Values for current and active power in excess of 20 A for which 500 Hz &lt; f ≤ 50 kHz. Values for current and active power in excess of 10 A for which 50 kHz &lt; f ≤ 100 kHz. Values for voltage and active power in excess of 750 V for which 30 kHz &lt; f ≤ 100 kHz.</li> </ul>			
	Effective measuring range	Voltage 1% to 150% of the range (1000 V range, up to 1000 V) Current 1% to 150% of the range Active power 0% to 225% of the range (when using 1000 V range, up to 150%) However, valid when the voltage and current fall within the effective measurement range.		
Maximum effective peak voltage	±600% of each voltage range However, for 300 V, 600 V, and 1000 V ranges, ±1500 V peak			
Maximum effective peak current	±600% of each current range However, for 20 A range, ±60 A peak			
Guaranteed accuracy period	1 year			
Post-adjustment accuracy guaranteed	6 months			
Temperature coefficient	Temperature and humidity range: 23°C±5°C (73°F±9°F), 80% RH or less Warm-up time: 30 minutes			
	Input: Sine wave input, power factor of 1, voltage to earth of 0 V, after zero-adjustment; within range in which the fundamental wave satisfies synchronization source conditions			

Range table (Power ranges)

Current/Voltage	6.0000 V	15.000 V	30.000 V	60.000 V	150.00 V	300.00 V	600.00 V	1.0000 kV
1.0000 mA	6.0000 mW	15.000 mW	30.000 mW	60.000 mW	150.00 mW	300.00 mW	600.00 mW	1.0000 W
2.0000 mA	12.000 mW	30.000 mW	60.000 mW	120.00 mW	300.00 mW	600.00 mW	1.2000 W	2.0000 W
5.0000 mA	30.000 mW	75.000 mW	150.00 mW	300.00 mW	750.00 mW	1.5000 W	3.0000 W	5.0000 W
10.000 mA	60.000 mW	150.00 mW	300.00 mW	600.00 mW	1.5000 W	3.0000 W	6.0000 W	10.000 W
20.000 mA	120.00 mW	300.00 mW	600.00 mW	1.2000 W	3.0000 W	6.0000 W	12.000 W	20.000 W
50.000 mA	300.00 mW	750.00 mW	1.5000 W	3.0000 W	7.5000 W	15.000 W	30.000 W	50.000 W
100.00 mA	600.00 mW	1.5000 W	3.0000 W	6.0000 W	15.000 W	30.000 W	60.000 W	100.00 W
200.00 mA	1.2000 W	3.0000 W	6.0000 W	12.000 W	30.000 W	60.000 W	120.00 W	200.00 W
500.00 mA	3.0000 W	7.5000 W	15.000 W	30.000 W	75.000 W	150.00 W	300.00 W	500.00 W
1.0000 A	6.0000 W	15.000 W	30.000 W	60.000 W	150.00 W	300.00 W	600.00 W	1.0000 kW
2.0000 A	12.000 W	30.000 W	60.000 W	120.00 W	300.00 W	600.00 W	1.2000 kW	2.0000 kW
5.0000 A	30.000 W	75.000 W	150.00 W	300.00 W	750.00 W	1.5000 kW	3.0000 kW	5.0000 kW
10.000 A	60.000 W	150.00 W	300.00 W	600.00 W	1.5000 kW	3.0000 kW	6.0000 kW	10.000 kW
20.000 A	120.00 W	300.00 W	600.00 W	1.2000 kW	3.0000 kW	6.0000 kW	12.000 kW	20.000 kW

Effect of power factor	±0.1% f.s. or less (45 to 66 Hz, at power factor = 0) Internal circuitry voltage/current phase difference: ±0.0573°
Effect of common mode voltage	±0.01% f.s. or less (600 V, 50 Hz/60 Hz, applied between input terminals and enclosure)
Effect of magnetic field	400 A/m, DC and 50 Hz/60 Hz magnetic field Voltage ±1.5% f.s. or less Current ±1.5% f.s. or less than or equal to the following value, whichever is greater 200 mA/ 500 mA/ 1 A/ 2 A/ 5 A/ 10 A/ 20 A range: ±20 mA 1 mA/ 2 mA/ 5 mA/ 10 mA/ 20 mA/ 50 mA/ 100 mA range: ±200 µA Active power ±3.0% f.s. or less than or equal to the following value, whichever is greater 200 mA/ 500 mA/ 1 A/ 2 A/ 5 A/ 10 A/ 20 A range: (Voltage influence quantity) × (±20 mA) 1 mA/ 2 mA/ 5 mA/ 10 mA/ 20 mA/ 50 mA/ 100 mA range: (Voltage influence quantity) × (±200 µA)
Effect of self-heating	With input of at least 15 A to current input terminals Current AC input signal ±(0.025+0.005×(I-15))% rdg. or less DC input signal 200 mA/ 500 mA/ 1 A/ 2 A/ 5 A/ 10 A/ 20 A range ±((0.025+0.005×(I-15))% rdg.+(0.5+0.1×(I-15))mA) or less 1 mA/ 2 mA/ 5 mA/ 10 mA/ 20 mA/ 50 mA/ 100 mA range ±((0.025+0.005×(I-15))% rdg.+(5+1×(I-15))µA) or less I: Current read value (A) Active power (above current influence quantity) × (voltage read value) or less  The effects of self-heating will continue to manifest themselves until the input resistance temperature falls, even if the current value is low.

### Voltage/ Current/ Active Power Measurement Specifications

Measurement types	Rectifiers: AC+DC, DC, AC, FND, AC+DC Umn
Effective measuring range	Voltage ±1% to ±150% of the range. However, up to ±1500 V peak value and 1000 V RMS value Current ±1% to ±150% of the range Active Power ±0% to ±225% of the range. However, valid when the voltage and current fall within the effective measurement range.
Display range	Voltage Up to ±152% of the range. However, zero-suppression when less than ±0.5% Current Up to ±152% of the range. However, zero-suppression when less than ±0.5% or less than ±9 µA. Active Power ±0% to ±231.04% of the range (no zero-suppression)
Polarity	Voltage/ Current Displayed when using DC rectifier Active Power Positive : Power consumption (no polarity display) Negative : generation or regenerated power

### Frequency Measurement Specifications

Number of measurement channels	2 (Voltage, current)
Measurement method	Calculated from input waveform period (reciprocal method)
Measurement ranges	100 Hz/ 500 Hz/ 5 kHz/ 100 kHz (linked to zero-cross filter)
Measurement accuracy	±0.1% rdg. ±1 dgt. However, for 1 mA range, ±0.2% rdg. ±1 dgt.
Effective measuring range	0.1 Hz to 100 kHz For sine wave input that is at least 20% of the measurement source's measurement range Measurement lower limit frequency setting: 0.1 sec. / 1 sec. / 10 sec. (linked to synchronization timeout setting)
Display format	0.1000 Hz to 9.9999 Hz, 9.900 Hz to 99.999 Hz, 99.00 Hz to 999.99 Hz, 0.9900 kHz to 9.9999 kHz, 9.900 kHz to 99.999 kHz, 99.00 kHz to 100.00 kHz

### Apparent Power/ Reactive Power/ Power Factor/ Phase Angle Measurement Specifications

Measurement types	Rectifiers Apparent Power/ Reactive Power/ Power Factor AC+DC, AC, FND, AC+DC Umn Phase Angle AC, FND
Effective measuring range	As per voltage, current, and active power effective measurement ranges

Display range	Apparent Power/ Reactive Power 0% to 231.04% of the range (no zero-suppression) Power Factor ±0.0000 to ±1.0000 Phase Angle +180.00 to -180.00
Polarity	Reactive Power/ Power Factor/ Phase Angle Polarity is assigned according to the lead/lag relationship of the voltage waveform rising edge and the current waveform rising edge. +: When current lags voltage (no polarity display) -: When current leads voltage

### Power Calculation Formulas

S : Apparent power	$S = U \times I$
Q : Reactive power	$Q = si \sqrt{S^2 - P^2}$
λ : Power factor	$\lambda = si I P/S I$
φ : Phase angle	$\phi = si I \cos^{-1} \lambda I$ (±90° to ±180°) $\phi = si I 180 - \cos^{-1} \lambda II$ (0° to ±90°)

U: Voltage, I: Current, P: Active Power, si: Polarity symbol (acquired based on voltage waveform and current waveform lead and lag)

### Voltage Waveform Peak Value/ Current Waveform Peak Value Measurement Specifications

Measurement method	Measures the voltage waveform's peak value (for both positive and negative polarity) based on sampled instantaneous voltage values.																																																
Range configuration	Voltage																																																
	<table border="1"> <thead> <tr> <th>Voltage range</th> <th>Voltage peak range</th> </tr> </thead> <tbody> <tr><td>6.0000 V</td><td>36.000 V</td></tr> <tr><td>15.000 V</td><td>90.000 V</td></tr> <tr><td>30.000 V</td><td>180.00 V</td></tr> <tr><td>60.000 V</td><td>360.00 V</td></tr> <tr><td>150.00 V</td><td>900.00 V</td></tr> <tr><td>300.00 V</td><td>1.8000 kV</td></tr> <tr><td>600.00 V</td><td>3.6000 kV</td></tr> <tr><td>1.0000 kV</td><td>6.0000 kV</td></tr> </tbody> </table>	Voltage range	Voltage peak range	6.0000 V	36.000 V	15.000 V	90.000 V	30.000 V	180.00 V	60.000 V	360.00 V	150.00 V	900.00 V	300.00 V	1.8000 kV	600.00 V	3.6000 kV	1.0000 kV	6.0000 kV	<table border="1"> <thead> <tr> <th>Current range</th> <th>Current peak range</th> </tr> </thead> <tbody> <tr><td>1.0000 mA</td><td>6.0000 mA</td></tr> <tr><td>2.0000 mA</td><td>12.000 mA</td></tr> <tr><td>5.0000 mA</td><td>30.000 mA</td></tr> <tr><td>10.000 mA</td><td>60.000 mA</td></tr> <tr><td>20.000 mA</td><td>120.00 mA</td></tr> <tr><td>50.000 mA</td><td>300.00 mA</td></tr> <tr><td>100.00 mA</td><td>600.00 mA</td></tr> <tr><td>200.00 mA</td><td>1.2000 A</td></tr> <tr><td>500.00 mA</td><td>3.0000 A</td></tr> <tr><td>1.0000 A</td><td>6.0000 A</td></tr> <tr><td>2.0000 A</td><td>12.000 A</td></tr> <tr><td>5.0000 A</td><td>30.000 A</td></tr> <tr><td>10.000 A</td><td>60.000 A</td></tr> <tr><td>20.000 A</td><td>120.00 A</td></tr> </tbody> </table>	Current range	Current peak range	1.0000 mA	6.0000 mA	2.0000 mA	12.000 mA	5.0000 mA	30.000 mA	10.000 mA	60.000 mA	20.000 mA	120.00 mA	50.000 mA	300.00 mA	100.00 mA	600.00 mA	200.00 mA	1.2000 A	500.00 mA	3.0000 A	1.0000 A	6.0000 A	2.0000 A	12.000 A	5.0000 A	30.000 A	10.000 A	60.000 A	20.000 A
Voltage range	Voltage peak range																																																
6.0000 V	36.000 V																																																
15.000 V	90.000 V																																																
30.000 V	180.00 V																																																
60.000 V	360.00 V																																																
150.00 V	900.00 V																																																
300.00 V	1.8000 kV																																																
600.00 V	3.6000 kV																																																
1.0000 kV	6.0000 kV																																																
Current range	Current peak range																																																
1.0000 mA	6.0000 mA																																																
2.0000 mA	12.000 mA																																																
5.0000 mA	30.000 mA																																																
10.000 mA	60.000 mA																																																
20.000 mA	120.00 mA																																																
50.000 mA	300.00 mA																																																
100.00 mA	600.00 mA																																																
200.00 mA	1.2000 A																																																
500.00 mA	3.0000 A																																																
1.0000 A	6.0000 A																																																
2.0000 A	12.000 A																																																
5.0000 A	30.000 A																																																
10.000 A	60.000 A																																																
20.000 A	120.00 A																																																
Measurement accuracy	±2.0% f.s. at DC and when 10 Hz ≤ f ≤ 1 kHz (f.s.: current peak range). Provided as reference value when 0.1 Hz ≤ f < 10 Hz and when 1 kHz < f. The above measurement accuracy is multiplied by 2 for the 1 mA range.																																																
Effective measuring range	±5% to ±100% of current peak range, however, up to ±60 A																																																
Display range	Up to ±102% of current peak range, however, the value 0 will be displayed if the current RMS value triggers the instrument's zero suppression function.																																																

### Voltage Crest Factor/Current Crest Factor Measurement Specifications

Measurement method	Calculates the ratio of the voltage waveform peak value to the voltage RMS value.
Effective measuring range	As per voltage and voltage waveform peak value, or current and current waveform peak value effective measurement ranges.
Display range	1.0000 to 612.00 (no polarity)

### Voltage Ripple Rate/ Current Ripple Rate Measurement Specifications

Measurement method	Calculates the AC component (peak to peak [peak width]) as a proportion of the voltage or current DC component.
Effective measuring range	As per voltage and voltage waveform peak value, or current and current waveform peak value effective measurement ranges.
Display range	0.00 to 500.00 (No polarity)



# Maximum Current Ratio Measurement Specifications (MCR)

Measurement method	Calculates the ratio of the current crest factor to the power factor. (MCR) = (Current Crest Factor) / (Power Factor)
Effective measuring range	As per power factor (voltage, current, active power) and current crest factor (current, current waveform peak value) effective measurement ranges.
Display range	1.0000 to 6.1200 M (no polarity)

## Synchronized control

Functions	The timing of calculations; display updates; data updates; integration start, stop, and reset events; display hold operation; key lock operation; and zero-adjustment operation for the slave PW3335 series is synchronized with the master PW3335 series. Synchronization with the PW3336 series and PW3337 series is also supported.
Terminal	BNC terminal × 1 (non-isolated)
Terminal name	External synchronization terminal (EXT.SYNC)
I/O settings	Off Synchronized control function off (signals input to the external synchronization terminal (EXT.SYNC) are ignored) In The external synchronization terminal (EXT.SYNC) is set to input, and a dedicated synchronization signal can be input (slave). Out The external synchronization terminal (EXT.SYNC) is set to output, and a dedicated synchronization signal can be output (master).
Number of units for which synchronized control can be performed	Up to 7 slaves per master (total of 8 units including the PW3336/PW3337 series)

## Functional Specifications

Auto-range (AUTO)	Automatically changes the voltage and current range according to the input.  Range up: The range is increased when input exceeds 150% of the range or when the peak is exceeded. Range down: The range is decreased when input falls below 15% of the range. However, the range is not decreased when the peak is exceeded at the lower range. The input level is monitored, and the range is switched over multiple ranges. Range select can be used to disable ranges so that they are not selected.																
Range select	Selects whether to enable (turn on) or disable (turn off) individual voltage and current ranges.  Enabled (use): Ranges can be selected with the range keys. Range switching occurs using auto-range operation. Range switching occurs during auto-range integration. Disabled (do not use): Ranges cannot be selected with the range keys. Range switching does not occur using auto-range operation. Range switching does not occur during auto-range integration.																
Zero-cross filter's threshold level	Sets the zero-cross filter's threshold level for voltage and current ranges. Set from 1% to 15% (in 1% intervals). Synchronization occurs when the percentage level set for each measurement range is exceeded.																
Averaging	Averages the voltage, current, active power, apparent power, and reactive power. (Other than harmonic measurement parameters.) The power factor and phase angle are calculated from averaged data. Averaging is not performed for parameters other than those listed above. Method: Simple averaging  Number of averaging iterations and display update interval <table border="1"> <thead> <tr> <th>Number of averaging iterations</th> <th>Display update interval</th> </tr> </thead> <tbody> <tr> <td>1 (OFF)</td> <td>200 ms</td> </tr> <tr> <td>2</td> <td>400 ms</td> </tr> <tr> <td>5</td> <td>1 s</td> </tr> <tr> <td>10</td> <td>2 s</td> </tr> <tr> <td>25</td> <td>5 s</td> </tr> <tr> <td>50</td> <td>10 s</td> </tr> <tr> <td>100</td> <td>20 s</td> </tr> </tbody> </table>	Number of averaging iterations	Display update interval	1 (OFF)	200 ms	2	400 ms	5	1 s	10	2 s	25	5 s	50	10 s	100	20 s
Number of averaging iterations	Display update interval																
1 (OFF)	200 ms																
2	400 ms																
5	1 s																
10	2 s																
25	5 s																
50	10 s																
100	20 s																
Scaling (VT, CT)	Applies user-defined VT and CT ratio settings to measured values. VT ratio setting range OFF (1.0), 0.001 to 1000 CT ratio setting range OFF (1.0), 0.001 to 1000																
Hold	<ul style="list-style-type: none"> <li>Stops display updates for all measured values and fixes the display values at that point in time.</li> <li>Measurement data acquired by communications is also fixed at that point in time.</li> <li>Internal calculations (including integration and integration elapsed time) will continue.</li> <li>Analog output and waveform output are not held</li> </ul>																

Maximum value/minimum value hold (MAX/MIN HOLD)	<ul style="list-style-type: none"> <li>Detects maximum and minimum measured values (except current integration, active power integration, integration elapsed time, time average current, and time average active power values) as well as maximum and minimum values for the voltage waveform peak and current waveform peak and holds them on the display.</li> <li>For data with polarity, display of the maximum value and minimum value for the data's absolute values is held (so that both positive and negative polarity values are shown). However, this does not apply to the voltage waveform peak value or the current waveform peak value.</li> <li>Internal calculations (including integration and integration elapsed time) will continue.</li> <li>The maximum and minimum values during integration are detected (maximum/minimum value measurement during the integration interval).</li> <li>Analog output and waveform output are not held.</li> </ul>
Zero Adjustment	Zeroes out the voltage and current input offset.
Key-lock	Disables key input in the measurement state, except for the KEY LOCK key.
Backup	Backs up settings and integration data if the instrument is turned off and if a power outage occurs.
System Reset	Initializes the instrument's settings.

## Integration Measurement Specifications

Integration operation modes	Switchable between fixed-range integration and auto-range integration.  Fixed-range integration Integration can be performed for all voltage and current ranges. The voltage and current ranges are fixed once integration starts. Auto-range integration Integration can be performed for all voltage ranges. The current is set to auto-range operation using ranges from 200 mA to 20 A. The integrated value for each range can be displayed by switching the current range (200 mA to 20 A) while integration is stopped.
Measurement items and display	Simultaneous integration of the following 6 parameters: Positive current integrated value (Ah+) Negative current integrated value (Ah-) Sum of current integrated values (Ah) Positive active power integrated value (Wh+) Negative active power integrated value (Wh-) Sum of active power integrated values (Wh)
Measurement types	Rectifiers: AC+DC, AC+DC Umn Current: Displays the result of integrating current RMS value data (display values) once every display update interval as an integrated value. Active power: Displays the result of integrating active power values by polarity calculated once every cycle for the selected synchronization source as integrated values. Rectifier: DC Displays the result of integrating instantaneous data obtained by sampling both current and active power by polarity as integrated values (these values are not integrated values for the DC component when active power contains both DC and AC components)
Integration time	1 min. to 10000 hr., settable in 1 min. blocks
Integration time accuracy	±0.01% rdg. ±1 dgt.
Integration measurement accuracy	(Current or active power measurement accuracy) + (±0.01% rdg. ±1 dgt.)
Effective measuring range	Until PEAK OVER U lamp or PEAK OVER I lamp lights up.
Display resolution	999999 (6 digits + decimal point)
Functions	<ul style="list-style-type: none"> <li>Stopping integration based on integration time setting (timer)</li> <li>Stopping/starting integration and resetting integrated values based on external control</li> <li>Displaying the integration elapsed time (displayed as TIME on panel display)</li> <li>Additional integration by repeatedly starting/stopping integration</li> <li>Backing up integrated values and the integration elapsed time during power outages</li> <li>Stopping integration when power returns</li> </ul>

## Time Average Current/ Time Average Active Power Measurement Specifications

Measurement method	Calculates the average by dividing the current or active power integrated value by the integration time.
Measurement accuracy	(Current or Active power measurement accuracy) + (±0.01% rdg. ±1 dgt.)
Effective measuring range	As per the current or active power integration effective measurement range.
Display range	Time Average Current ±0% to ±612% of the range (Has polarity when using the DC rectifier.) Time Average Active Power ±0% to ±3745.4% of the range (Has polarity)


## Harmonic Measurement Specifications

Measurement method	Zero-cross simultaneous calculation method Uniform thinning between zero-cross events after processing with a digital antialiasing filter Interpolation calculations (Lagrange interpolation) When the synchronization frequency falls within the 45 Hz to 66 Hz range: IEC 61000-4-7:2002 compliant Gaps and overlaps may occur if the measurement frequency is not 50 Hz or 60 Hz. When the synchronization frequency falls outside the 45 Hz to 66 Hz range: No gaps or overlap will occur.	
Synchronization source	Conforms to synchronization source (SYNC) for the basic measurement specifications.	
Measurement items	Harmonic voltage RMS value Harmonic voltage phase angle Harmonic current content percentage Harmonic active power Harmonic active power content percentage Harmonic voltage current phase difference Total harmonic voltage distortion Fundamental wave voltage Fundamental wave active power Fundamental wave reactive power Fundamental wave voltage current phase difference (The following parameters can be downloaded as data with communications) Harmonic voltage phase angle Harmonic voltage current phase difference	Harmonic voltage content percentage Harmonic current RMS value Harmonic current phase angle Harmonic current phase angle Total harmonic current distortion Fundamental wave current Fundamental wave apparent power Fundamental wave power factor
FFT processing	FFT processing word length : 32 bits Number of FFT points : 4096 points	
Window function	Rectangular	
Analysis window width	45 Hz ≤ f < 56 Hz : 178.57 ms to 222.22 ms (10 cycles) 56 Hz ≤ f < 66 Hz : 181.82 ms to 214.29 ms (12 cycles) Frequencies other than the above : 185.92 ms to 214.08 ms	
Data update rate	Depends on window width.	
Maximum analysis order	Synchronization frequency (f) range	Analysis order
	10 Hz ≤ f < 45 Hz	50th
	45 Hz ≤ f < 56 Hz	50th
	56 Hz ≤ f ≤ 66 Hz	50th
	66 Hz < f ≤ 100 Hz	50th
	100 Hz < f ≤ 200 Hz	40th
	200 Hz < f ≤ 300 Hz	25th
	300 Hz < f ≤ 500 Hz	15th
	500 Hz < f ≤ 640 Hz	11th
Analysis order upper limit setting	2nd to 50th	
Measurement accuracy	f.s.: Measurement range	
	Frequency (f)	Voltage, Current, Active power
	DC	±0.4% rdg. ±0.2% f.s.
	10 Hz ≤ f < 30 Hz	±0.4% rdg. ±0.2% f.s.
	30 Hz ≤ f ≤ 400 Hz	±0.3% rdg. ±0.1% f.s.
	400 Hz < f ≤ 1 kHz	±0.4% rdg. ±0.2% f.s.
	1 kHz < f ≤ 5 kHz	±1.0% rdg. ±0.5% f.s.
	5 kHz < f ≤ 8 kHz	±4.0% rdg. ±1.0% f.s.
	<ul style="list-style-type: none"> <li>When using the 1 mA / 2 mA range: Add ±1 μA to 10 Hz to 8 kHz measurement accuracy for current. Add (±1 μA) × (voltage read value) to 10 Hz to 8 kHz measurement accuracy for active power.</li> <li>When using the 200 mA / 500 mA / 1 A / 2 A / 5 A / 10 A / 20 A range: Add ±1 mA to DC measurement accuracy for current. Add (±1 mA) × (voltage read value) to DC measurement accuracy for active power.</li> <li>When using the 1 mA / 2 mA / 5 mA / 10 mA / 20 mA / 50 mA / 100 mA range: Add ±10 μA to DC measurement accuracy for current. Add (±10 μA) × (voltage read value) to DC measurement accuracy for active power.</li> </ul>	

## Display Specifications

Display	7-segment LED
Number of display parameters	4 (display area a, b, c, and d)
Display resolution	Other than integrated values: 99999 count (5 digits) Integrated values: 999999 count (6 digits)
Display update rate	200 ms ±50 ms (approx. 5 updates per sec.) to 20 s (varies with number of averaging iterations setting)

## External Current Sensor Input Specifications (PW3335-03 and PW3335-04)

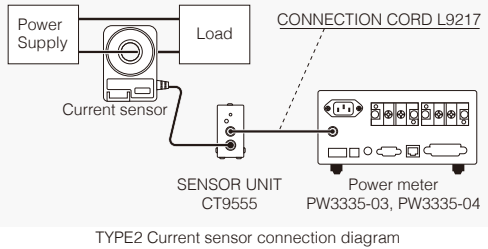Terminal	Isolated BNC terminals																																																																				
Current sensor type switching	Off / TYPE.1 / TYPE.2 When set to off, input from the external current sensor input terminal is ignored.																																																																				
Current sensor options	Supported current sensors  TYPE.1 (Can be directly connected) 9660 CLAMP ON SENSOR (100 A AC) 9661 CLAMP ON SENSOR (500 A AC) 9669 CLAMP ON SENSOR (1000 A AC) CT9667-01/ -02/ -03 AC FLEXIBLE CURRENT SENSOR (500A/ 5000 A AC)  TYPE.2 (Requires Sensor Unit CT9555 and Connection Cable L9217) CT6862-05 AC/DC CURRENT SENSOR (50 A AC/DC) CT6863-05 AC/DC CURRENT SENSOR (200 A AC/DC) 9709-05 AC/DC CURRENT SENSOR (500 A AC/DC) CT6865-05 AC/DC CURRENT SENSOR (1000 A AC/DC) CT6841-05 AC/DC CURRENT PROBE (20 A AC/DC) CT6843-05 AC/DC CURRENT PROBE (200 A AC/DC) CT6844-05 AC/DC CURRENT PROBE (500 A AC/DC) CT6845-05 AC/DC CURRENT PROBE (500 A AC/DC) CT6846-05 AC/DC CURRENT PROBE (1000 A AC/DC) 9272-05 CLAMP ON SENSOR (20 A / 200 A AC)																																																																				
	 <p>TYPE2 Current sensor connection diagram</p>																																																																				
Current measurement range	Auto/ 1 A / 2 A / 5 A (range noted on panel) Can be read directly by manually setting the CT ratio.																																																																				
Constraints	Auto-range integration not supported.																																																																				
Power range configuration	Depends on the combination of voltage and current ranges; from 24.000 W to 5.0000 MW (also applies to VA, var)																																																																				
Measurement accuracy	<table border="1"> <thead> <tr> <th colspan="4">Current/ Active Power</th> </tr> <tr> <th>Frequency ( f )</th> <th>Input &lt; 50% f.s.</th> <th>50% f.s. ≤ Input &lt; 100% f.s.</th> <th>100% f.s. ≤ Input</th> </tr> </thead> <tbody> <tr> <td>DC</td> <td>±0.1%rdg.±0.2% f.s.</td> <td>±0.1%rdg.±0.2% f.s.</td> <td>±0.3%rdg.</td> </tr> <tr> <td>0.1Hz≤f&lt;16Hz</td> <td>±0.1%rdg.±0.2% f.s.</td> <td>±0.3%rdg.</td> <td>±0.3%rdg.</td> </tr> <tr> <td>16Hz≤f&lt;45Hz</td> <td>±0.1%rdg.±0.2% f.s.</td> <td>±0.3%rdg.</td> <td>±0.3%rdg.</td> </tr> <tr> <td>45Hz≤f≤66Hz</td> <td>±0.1%rdg.±0.1% f.s.</td> <td>±0.2%rdg.</td> <td>±0.2%rdg.</td> </tr> <tr> <td>66Hz&lt;f≤500Hz</td> <td>±0.1%rdg.±0.2% f.s.</td> <td>±0.3%rdg.</td> <td>±0.3%rdg.</td> </tr> <tr> <td>500Hz&lt;f≤1kHz</td> <td>±0.1%rdg.±0.2% f.s.</td> <td>±0.3%rdg.</td> <td>±0.3%rdg.</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th colspan="4">Current</th> </tr> <tr> <th>Frequency ( f )</th> <th>Input &lt; 50% f.s.</th> <th>50% f.s. ≤ Input &lt; 100% f.s.</th> <th>100% f.s. ≤ Input</th> </tr> </thead> <tbody> <tr> <td>1kHz&lt;f≤10kHz</td> <td>±(0.03+0.07×F)%rdg. ±0.2% f.s.</td> <td>±(0.23+0.07×F)%rdg.</td> <td>±(0.23+0.07×F)%rdg.</td> </tr> <tr> <td>10kHz&lt;f≤100kHz</td> <td>±(0.3+0.04×F)%rdg. ±0.3% f.s.</td> <td>±(0.6+0.04×F)%rdg.</td> <td>±(0.6+0.04×F)%rdg.</td> </tr> </tbody> </table> <table border="1"> <thead> <tr> <th colspan="4">Active Power</th> </tr> <tr> <th>Frequency ( f )</th> <th>Input &lt; 50% f.s.</th> <th>50% f.s. ≤ Input &lt; 100% f.s.</th> <th>100% f.s. ≤ Input</th> </tr> </thead> <tbody> <tr> <td>1kHz&lt;f≤10kHz</td> <td>±(0.03+0.07×F)%rdg. ±0.2% f.s.</td> <td>±(0.23+0.07×F)%rdg.</td> <td>±(0.23+0.07×F)%rdg.</td> </tr> <tr> <td>10kHz&lt;f≤50kHz</td> <td>±(0.07×F)%rdg. ±0.3% f.s.</td> <td>±(0.3+0.07×F)%rdg.</td> <td>±(0.3+0.07×F)%rdg.</td> </tr> <tr> <td>50kHz&lt;f≤100kHz</td> <td>±(0.6+0.07×F)%rdg. ±0.3% f.s.</td> <td>±(0.9+0.07×F)%rdg.</td> <td>±(0.9+0.07×F)%rdg.</td> </tr> </tbody> </table>	Current/ Active Power				Frequency ( f )	Input < 50% f.s.	50% f.s. ≤ Input < 100% f.s.	100% f.s. ≤ Input	DC	±0.1%rdg.±0.2% f.s.	±0.1%rdg.±0.2% f.s.	±0.3%rdg.	0.1Hz≤f<16Hz	±0.1%rdg.±0.2% f.s.	±0.3%rdg.	±0.3%rdg.	16Hz≤f<45Hz	±0.1%rdg.±0.2% f.s.	±0.3%rdg.	±0.3%rdg.	45Hz≤f≤66Hz	±0.1%rdg.±0.1% f.s.	±0.2%rdg.	±0.2%rdg.	66Hz<f≤500Hz	±0.1%rdg.±0.2% f.s.	±0.3%rdg.	±0.3%rdg.	500Hz<f≤1kHz	±0.1%rdg.±0.2% f.s.	±0.3%rdg.	±0.3%rdg.	Current				Frequency ( f )	Input < 50% f.s.	50% f.s. ≤ Input < 100% f.s.	100% f.s. ≤ Input	1kHz<f≤10kHz	±(0.03+0.07×F)%rdg. ±0.2% f.s.	±(0.23+0.07×F)%rdg.	±(0.23+0.07×F)%rdg.	10kHz<f≤100kHz	±(0.3+0.04×F)%rdg. ±0.3% f.s.	±(0.6+0.04×F)%rdg.	±(0.6+0.04×F)%rdg.	Active Power				Frequency ( f )	Input < 50% f.s.	50% f.s. ≤ Input < 100% f.s.	100% f.s. ≤ Input	1kHz<f≤10kHz	±(0.03+0.07×F)%rdg. ±0.2% f.s.	±(0.23+0.07×F)%rdg.	±(0.23+0.07×F)%rdg.	10kHz<f≤50kHz	±(0.07×F)%rdg. ±0.3% f.s.	±(0.3+0.07×F)%rdg.	±(0.3+0.07×F)%rdg.	50kHz<f≤100kHz	±(0.6+0.07×F)%rdg. ±0.3% f.s.	±(0.9+0.07×F)%rdg.	±(0.9+0.07×F)%rdg.
Current/ Active Power																																																																					
Frequency ( f )	Input < 50% f.s.	50% f.s. ≤ Input < 100% f.s.	100% f.s. ≤ Input																																																																		
DC	±0.1%rdg.±0.2% f.s.	±0.1%rdg.±0.2% f.s.	±0.3%rdg.																																																																		
0.1Hz≤f<16Hz	±0.1%rdg.±0.2% f.s.	±0.3%rdg.	±0.3%rdg.																																																																		
16Hz≤f<45Hz	±0.1%rdg.±0.2% f.s.	±0.3%rdg.	±0.3%rdg.																																																																		
45Hz≤f≤66Hz	±0.1%rdg.±0.1% f.s.	±0.2%rdg.	±0.2%rdg.																																																																		
66Hz<f≤500Hz	±0.1%rdg.±0.2% f.s.	±0.3%rdg.	±0.3%rdg.																																																																		
500Hz<f≤1kHz	±0.1%rdg.±0.2% f.s.	±0.3%rdg.	±0.3%rdg.																																																																		
Current																																																																					
Frequency ( f )	Input < 50% f.s.	50% f.s. ≤ Input < 100% f.s.	100% f.s. ≤ Input																																																																		
1kHz<f≤10kHz	±(0.03+0.07×F)%rdg. ±0.2% f.s.	±(0.23+0.07×F)%rdg.	±(0.23+0.07×F)%rdg.																																																																		
10kHz<f≤100kHz	±(0.3+0.04×F)%rdg. ±0.3% f.s.	±(0.6+0.04×F)%rdg.	±(0.6+0.04×F)%rdg.																																																																		
Active Power																																																																					
Frequency ( f )	Input < 50% f.s.	50% f.s. ≤ Input < 100% f.s.	100% f.s. ≤ Input																																																																		
1kHz<f≤10kHz	±(0.03+0.07×F)%rdg. ±0.2% f.s.	±(0.23+0.07×F)%rdg.	±(0.23+0.07×F)%rdg.																																																																		
10kHz<f≤50kHz	±(0.07×F)%rdg. ±0.3% f.s.	±(0.3+0.07×F)%rdg.	±(0.3+0.07×F)%rdg.																																																																		
50kHz<f≤100kHz	±(0.6+0.07×F)%rdg. ±0.3% f.s.	±(0.9+0.07×F)%rdg.	±(0.9+0.07×F)%rdg.																																																																		
	<ul style="list-style-type: none"> <li>Values for f.s. depend on measurement ranges.</li> <li>“F” in the tables refers to the frequency in kHz.</li> <li>To obtain the current or active power accuracy, add the current sensor's accuracy to the above current and active power accuracy figures.</li> <li>The effective measurement range and frequency characteristics conform to the current sensor's specifications.</li> <li>The following input are considered reference values: Values for voltage, current, and active power for which 0.1 Hz ≤ f &lt; 10 Hz. Values for voltage and active power in excess of 220 V for which 10 Hz ≤ f &lt; 16 Hz. Values for voltage and active power in excess of 750 V for which 30 kHz &lt; f ≤ 100 kHz.</li> <li>When using the CT684x-05 series, add ±2 mV to the CT684x-05 series accuracy after performing CT684x-05 series zero adjustment using the 1 A range noted on the panel.</li> </ul>																																																																				

Temperature coefficient	Current, active power: $\pm 0.08\% \text{f.s./}^\circ\text{C}$ or less (instrument temperature coefficient; f.s.: instrument measurement range) Add current sensor temperature coefficient to above.													
Effect of power factor	Instrument: $\pm 0.15\% \text{f.s.}$ or less (45 to 66 Hz with power factor = 0) Internal circuit voltage/current phase difference: $\pm 0.0859^\circ$ Add the current sensor phase accuracy to the internal circuit voltage/current phase difference noted above.													
Current waveform peak value measurement specifications	$\pm 2.0\%$ at DC or $10 \text{ Hz} \leq f \leq 1 \text{ kHz}$ (f.s.: current peak range) Add the current sensor accuracy to the above.													
Harmonic measurement accuracy	External current sensor input instrument measurement accuracy only													
	<table border="1"> <thead> <tr> <th>Frequency (f)</th> <th>Voltage, Current, Active power</th> </tr> </thead> <tbody> <tr> <td>DC</td> <td><math>\pm 0.4\% \text{ rdg.} \pm 0.2\% \text{f.s.}</math></td> </tr> <tr> <td><math>10 \text{ Hz} \leq f &lt; 30 \text{ Hz}</math></td> <td><math>\pm 0.4\% \text{ rdg.} \pm 0.2\% \text{f.s.}</math></td> </tr> <tr> <td><math>30 \text{ Hz} \leq f \leq 400 \text{ Hz}</math></td> <td><math>\pm 0.3\% \text{ rdg.} \pm 0.1\% \text{f.s.}</math></td> </tr> <tr> <td><math>400 \text{ Hz} &lt; f \leq 1 \text{ kHz}</math></td> <td><math>\pm 0.4\% \text{ rdg.} \pm 0.2\% \text{f.s.}</math></td> </tr> <tr> <td><math>1 \text{ kHz} &lt; f \leq 5 \text{ kHz}</math></td> <td><math>\pm 1.0\% \text{ rdg.} \pm 0.5\% \text{f.s.}</math></td> </tr> <tr> <td><math>5 \text{ kHz} &lt; f \leq 8 \text{ kHz}</math></td> <td><math>\pm 4.0\% \text{ rdg.} \pm 1.0\% \text{f.s.}</math></td> </tr> </tbody> </table> <ul style="list-style-type: none"> <li>• Values for f.s. depend on measurement ranges.</li> <li>• To obtain the current or active power accuracy, add the current sensor's accuracy to the above current and active power accuracy figures.</li> <li>• When using the CT684x-05 series, add <math>\pm 2 \text{ mV}</math> to the CT684x-05 series accuracy after performing CT684x-05 series zero adjustment using the 1 A range noted on the panel.</li> </ul>	Frequency (f)	Voltage, Current, Active power	DC	$\pm 0.4\% \text{ rdg.} \pm 0.2\% \text{f.s.}$	$10 \text{ Hz} \leq f < 30 \text{ Hz}$	$\pm 0.4\% \text{ rdg.} \pm 0.2\% \text{f.s.}$	$30 \text{ Hz} \leq f \leq 400 \text{ Hz}$	$\pm 0.3\% \text{ rdg.} \pm 0.1\% \text{f.s.}$	$400 \text{ Hz} < f \leq 1 \text{ kHz}$	$\pm 0.4\% \text{ rdg.} \pm 0.2\% \text{f.s.}$	$1 \text{ kHz} < f \leq 5 \text{ kHz}$	$\pm 1.0\% \text{ rdg.} \pm 0.5\% \text{f.s.}$	$5 \text{ kHz} < f \leq 8 \text{ kHz}$
Frequency (f)	Voltage, Current, Active power													
DC	$\pm 0.4\% \text{ rdg.} \pm 0.2\% \text{f.s.}$													
$10 \text{ Hz} \leq f < 30 \text{ Hz}$	$\pm 0.4\% \text{ rdg.} \pm 0.2\% \text{f.s.}$													
$30 \text{ Hz} \leq f \leq 400 \text{ Hz}$	$\pm 0.3\% \text{ rdg.} \pm 0.1\% \text{f.s.}$													
$400 \text{ Hz} < f \leq 1 \text{ kHz}$	$\pm 0.4\% \text{ rdg.} \pm 0.2\% \text{f.s.}$													
$1 \text{ kHz} < f \leq 5 \text{ kHz}$	$\pm 1.0\% \text{ rdg.} \pm 0.5\% \text{f.s.}$													
$5 \text{ kHz} < f \leq 8 \text{ kHz}$	$\pm 4.0\% \text{ rdg.} \pm 1.0\% \text{f.s.}$													

### D/A Output Specifications (PW3335-02 and PW3335-04)

Number of output channels	7 channels
Configuration	16-bit D/A converter (polarity + 15 bits)
Output voltage	The output level, output speed, and waveform output can be selected. Level output 2 Vf.s. or 5 Vf.s., linked to display updates High-speed level output 2 Vf.s. or 5 Vf.s., linked to synchronization interval Waveform output 1 Vf.s., linked to sampling
Output parameters	Output parameters for all channels Available selections vary with the output parameter.  Level output/ High-speed level output/ Waveform output Voltage, current, active power Only Level output Apparent power, reactive power, power factor, phase angle, total harmonic voltage distortion, total harmonic current distortion, voltage ripple rate, current ripple rate, voltage crest factor, current crest factor, time average current, time average active power, maximum current ratio Only Level output 5 Vf.s. Frequency, current integration, active power integration  The rectifier can be selected. Harmonic-order output is not supported.
Output accuracy	f.s.: Relative to the output voltage rated value for each output parameter Level output (Output parameter measurement accuracy) + ( $\pm 0.2\% \text{f.s.}$ ) High-speed level output (Output parameter measurement accuracy) + ( $\pm 0.2\% \text{f.s.}$ ) Waveform output (Output parameter measurement accuracy) + ( $\pm 1.0\% \text{f.s.}$ )
Output frequency band	Waveform output, high-speed level output At DC or 10 Hz to 30 kHz, accuracy is as defined above.
Maximum output voltage	Approx. $\pm 12 \text{ V DC}$
Output update rate	Level output Same as the data update period. High-speed level output AC Updated once every cycle for the input waveform set as the synchronization source. However, voltage and current are only updated once every cycle for input signals from 45 to 66 Hz. Waveform output Approx. $1.43 \mu\text{s}$ (approx. 700 kHz)
Response time	Level output 0.6 sec. or less High-speed level output 2 ms or less Waveform output 0.2 ms or less
Temperature coefficient	$\pm 0.05\% \text{f.s./}^\circ\text{C}$ or less
Output resistance	Approx. $100 \Omega$

### External control

Functions	Integration start/stop, integration reset and hold via external control
Input signal level	0 to 5 V (high-speed CMOS level) or shorted [Lo]/ open [Hi]

### GP-IB interface (PW3335-01 and PW3335-04)

Method	Compliant with IEEE488.1 1987, in reference to IEEE488.2 1987 Interface functions SH1, AH1, T6, L4, SR1, RL1, PP0, DC1, DT1, C0
Address	00 to 30

### RS-232C interface (PW3335, PW3335-02, PW3335-03, and PW3335-04)

Connector	D-sub 9-pin connector $\times 1$
Communication method	Full duplex, Start-stop synchronization Stop bits: 1 (fixed) Data length: 8 (fixed) Parity: None
Communication speed	9600 bps/ 38400 bps

### LAN interface

Connector	RJ-45 connector $\times 1$
Electrical specifications	Compliant with IEEE802.3
Transmission method	10Base-T/ 100Base-TX (automatic detection)
Protocol	TCP/ IP
Functions	HTTP server (remote operation, firmware updates) Dedicated ports (command control, data transfer) Remote control by controller

### General Specifications

Product warranty period	1 year
Operating environment	Indoors, altitude up to 2000 m (6562 ft.), pollution degree 2
Operating temperature and humidity	$0^\circ\text{C}$ to $40^\circ\text{C}$ ( $32^\circ\text{F}$ to $104^\circ\text{F}$ ), 80% RH or less (no condensation)
Storage temperature and humidity	$-10^\circ\text{C}$ to $50^\circ\text{C}$ ( $14^\circ\text{F}$ to $122^\circ\text{F}$ ), 80% RH or less (no condensation)
Dielectric strength	4290 V rms AC (current sensitivity: 1 mA) Between the voltage input terminals and a connection consisting of chassis, interfaces, and output terminals Between the current input terminals and a connection consisting of chassis, interfaces, and output terminals Between the voltage input terminals and current input terminals
Maximum rated voltage to earth	Voltage input terminal, Current input terminal Measurement category III 600 V (anticipated transient overvoltage: 6000 V) Measurement category II 1000 V (anticipated transient overvoltage: 6000 V)
Maximum input voltage	Between the voltage input terminals U and $\pm 1000 \text{ V}$ , $\pm 1500 \text{ V peak}$
Maximum input current	Between the current input terminals I and $\pm 200 \text{ mA}$ to $20 \text{ A}$ range $30 \text{ A}$ , $\pm 100 \text{ A peak}$ $1 \text{ mA}$ to $100 \text{ mA}$ range $20 \text{ A}$ , $\pm 30 \text{ A peak}$
Applicable Standards	Safety EN61010 EMC EN61326 Class A EN61000-3-2 EN61000-3-3
Rated supply voltage	100 V AC to 240 V AC 50 Hz/60 Hz
Maximum rated power	30 VA or less
Dimensions	Approx. $210\text{W} \times 100\text{H} \times 245\text{D mm}$ ( $8.27\text{''W} \times 3.94\text{''H} \times 9.65\text{''D}$ ) (excluding protrusions)
Mass	Approx. 3 kg (105.8 oz.)
Accessories	Instruction manual $\times 1$ Power cord $\times 1$ Voltage and current input terminal safety cover $\times 2$



The Right Source For Your Test & Measurement Needs

8715 Mesa Point Terrace San Diego, CA 92154  
Toll Free: 1.866.363.6634 Tel: 1.619.429.4545 Fax: 1.619.374.7012  
Email: sales@calright.com http://www.calright.com

# Model : POWER METER PW3335



Model (Order Cord)	Harmonics measurement	Synchronous control	LAN	RS-232C	GP-IB	D/A output	Current sensor input
PW3335	✓	✓	✓	✓	—	—	—
PW3335-01	✓	✓	✓	—	✓	—	—
PW3335-02	✓	✓	✓	✓	—	✓	—
PW3335-03	✓	✓	✓	✓	—	—	✓
PW3335-04	✓	✓	✓	✓	✓	✓	✓

Accessories : Instruction manual ×1, Power cord ×1, Voltage and current input terminal safety cover ×2

✓ : available  
— : not available

## Options

Current measurement options [Type 1] Can be directly connected to the current sensor input terminals on the PW3335-03/ PW3335-04



**CLAMP ON SENSOR 9660**  
100 A AC, φ15 mm(0.59"), 40 Hz to 5 kHz  
±0.3%rdg.±0.02%f.s. (Amplitude accuracy 45 Hz to 66 Hz)  
±1° or less (Phase accuracy 45 Hz to 66 Hz)



**CLAMP ON SENSOR 9661**  
500 A AC, φ46 mm(1.81"), 40 Hz to 5 kHz  
±0.3%rdg.±0.01%f.s. (Amplitude accuracy 45 Hz to 66 Hz)  
±0.5° or less (Phase accuracy 45 Hz to 66 Hz)



**CLAMP ON SENSOR 9669**  
1000 A AC, φ55mm(2.17"), 80 × 20 mm (3.15" × 0.79") busbar, 40 Hz to 5 kHz  
±1.0%rdg.±0.01%f.s. (Amplitude accuracy 45 Hz to 66 Hz)  
±1° or less (Phase accuracy 45 Hz to 66 Hz)



**CLAMP ON SENSOR CT9667-01, CT9667-02, CT9667-03**  
500 A /5000 A AC Switchable, φ100mm to φ254 mm (3.94" to 10"), 10 Hz to 20 kHz  
±2.0%rdg.±0.3%f.s. (Amplitude accuracy 45 Hz to 66 Hz)  
±1° or less (Phase accuracy 45 Hz to 66 Hz)  
Power supply : LR6 alkaline battery ×2, or AC Adapter (option)  
Option : AC ADAPTER 9445-02 (universal 100 V to 240 VAC /for USA)  
AC ADAPTER 9445-03 (universal 100 V to 240 VAC /for Europe)

Current measurement options [Type 2] **Requires Sensor Unit CT9555 and Connection Cable L9217 to be connected to the current sensor input terminals on the PW3335-03/ PW3335-04**

### 200 A or lower



**AC/DC CURRENT SENSOR CT6862-05**  
50 A AC/DC, pass-through type, φ24 mm(0.94"), DC to 1 MHz  
±0.05%rdg.±0.01%f.s. (Amplitude accuracy 16 Hz to 400 Hz)  
±0.2° or less (Phase accuracy 16 Hz to 400 Hz)  
Power supply : SENSOR UNIT CT9555 (option)



**AC/DC CURRENT SENSOR CT6863-05**  
200 A AC/DC, pass-through type, φ24 mm(0.94"), DC to 500 kHz  
±0.05%rdg.±0.01%f.s. (Amplitude accuracy 16 Hz to 400 Hz)  
±0.2° or less (Phase accuracy 16 Hz to 400 Hz)  
Power supply : SENSOR UNIT CT9555 (option)



**AC/DC CURRENT PROBE CT6841-05**  
20 A AC/DC, clamp-on type, φ20 mm(0.79"), DC to 1 MHz  
±0.3%rdg.±0.01%f.s. (Amplitude accuracy DC < f ≤ 100 Hz)  
±0.1° or less (Phase accuracy DC < f ≤ 100 Hz)  
Power supply : SENSOR UNIT CT9555 (option)



**AC/DC CURRENT PROBE CT6843-05**  
200 A AC/DC, clamp-on type, φ20 mm(0.79"), DC to 500 kHz  
±0.3%rdg.±0.01%f.s. (Amplitude accuracy DC < f ≤ 100 Hz)  
±0.1° or less (Phase accuracy DC < f ≤ 100 Hz)  
Power supply : SENSOR UNIT CT9555 (option)



**CLAMP ON SENSOR 9272-05 (Scheduled for release in 2017)**  
20 A / 200 A AC Switchable, clamp-on type, φ46 mm(1.81"),  
1 Hz to 100 kHz  
±0.3%rdg.±0.01%f.s. (Amplitude accuracy 45 Hz to 66 Hz)  
±0.2° or less (Phase accuracy 45 Hz to 66 Hz)  
Power supply : SENSOR UNIT CT9555 (option)

### 500 A or lower



**AC/DC CURRENT SENSOR 9709-05**  
500 A AC/DC, pass-through type, φ36 mm(1.42"), DC to 100 kHz  
±0.05%rdg.±0.01%f.s. (Amplitude accuracy 45 Hz to 66 Hz)  
±0.2° or less (Phase accuracy 45 Hz to 66 Hz)  
Power supply : SENSOR UNIT CT9555 (option)



**AC/DC CURRENT PROBE CT6844-05**  
500 A AC/DC, clamp-on type, φ20 mm(0.79"), DC to 200 kHz  
±0.3%rdg.±0.01%f.s. (Amplitude accuracy DC < f ≤ 100 Hz)  
±0.1° or less (Phase accuracy DC < f ≤ 100 Hz)  
Power supply : SENSOR UNIT CT9555 (option)



**AC/DC CURRENT PROBE CT6845-05**  
500 A AC/DC, clamp-on type, φ50 mm(1.97"), DC to 100 kHz  
±0.3%rdg.±0.01%f.s. (Amplitude accuracy DC < f ≤ 100 Hz)  
±0.1° or less (Phase accuracy DC < f ≤ 100 Hz)  
Power supply : SENSOR UNIT CT9555 (option)

### 1000 A or lower



**AC/DC CURRENT SENSOR CT6865-05**  
1000 A AC/DC, pass-through type, φ36 mm(1.42"), DC to 20 kHz  
±0.05%rdg.±0.01%f.s. (Amplitude accuracy 16 Hz to 66 Hz)  
±0.2° or less (Phase accuracy 16 Hz to 66 Hz)  
Power supply : SENSOR UNIT CT9555 (option)



**AC/DC CURRENT PROBE CT6846-05**  
1000 A AC/DC, clamp-on type, φ50 mm(1.97"), DC to 20 kHz  
±0.3%rdg.±0.01%f.s. (Amplitude accuracy DC < f ≤ 100 Hz)  
±0.1° or less (Phase accuracy DC < f ≤ 100 Hz)  
Power supply : SENSOR UNIT CT9555 (option)

## Type 2 Current sensor options



**SENSOR UNIT CT9555**  
POWER SUPPLY 100 V to 240 V AC (50Hz/ 60Hz)



**CONNECTION CORD L9217**  
For sensor output, Isolated BNC to isolated BNC  
Cord length: 1.6 m (5.25 ft) length

## Communications and control options



**RS-232C CABLE 9637**  
Cable length: 1.8 m (5.91 ft)  
9pin to 9pin



**RS-232C CABLE 9638**  
Cable length: 1.8 m (5.91 ft)  
9pin to 25pin



**GP-IB CONNECTOR CABLE 9151-02**  
Cable length: 2 m (6.56 ft)



**LAN CABLE 9642**  
Cable length: 5 m (16.41 ft)  
supplied with straight to cross conversion cable



**CONNECTION CORD 9165**  
For synchronized control  
Cable length: 1.5 m (4.92 ft),  
metal BNC to metal BNC

Note: Company names and Product names appearing in this catalog are trademarks or registered trademarks of various companies.